

Technical Sheet (US)

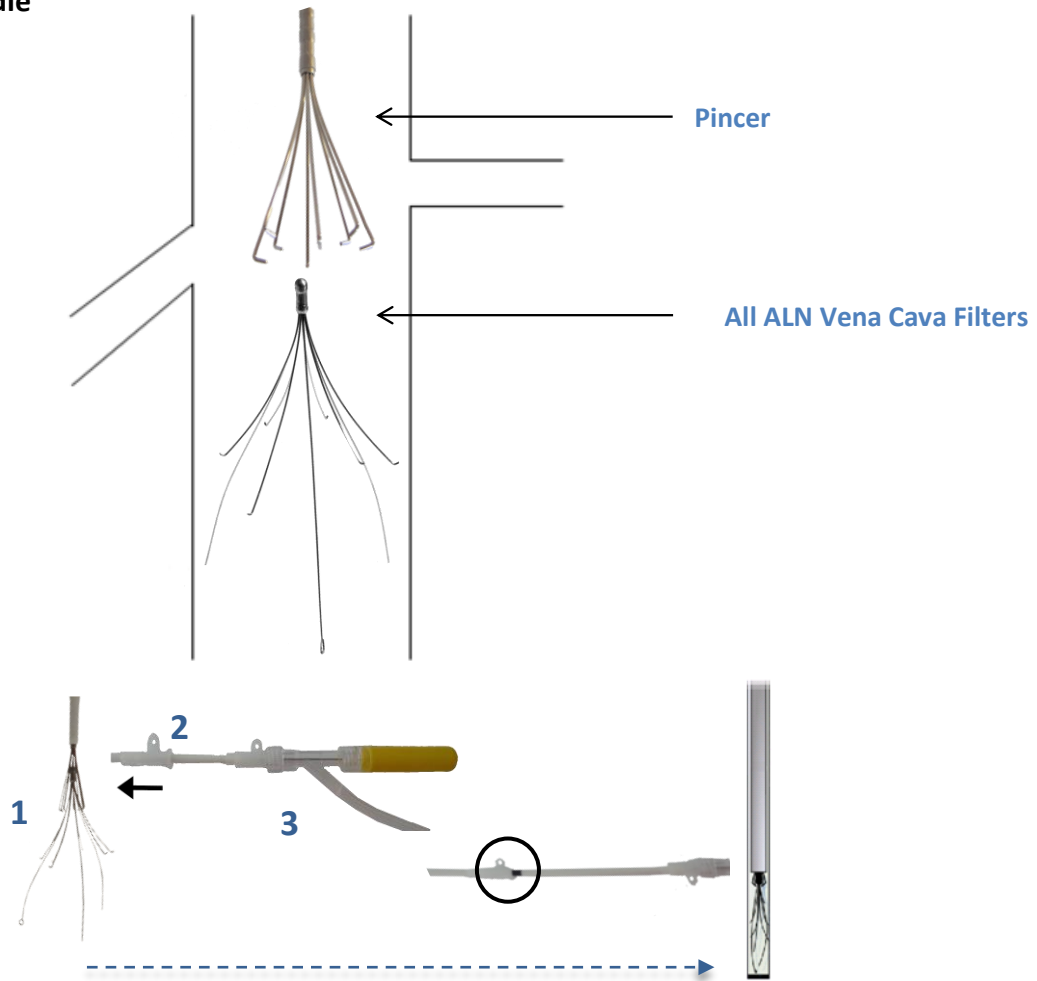
The ALN Extraction and/or Repositioning Kits

ALN Straight RS & ALN Pre-curved RS


- Only by jugular approach
- Pincer system: specially designed for the removal of all ALN Vena Cava Filters
- CE Mark 0297
- FDA Approved

The ALN Extraction and/or repositioning kits ALN STRAIGHT RS and ALN PRE-CURVED RS contain:

- ✓ A **Pincer catheter** (7F catheter with 2 black markers + pincer with 8 strands + 3-ways stop cock)
- ✓ An **introduction system** (dilator, 9F catheter with a radio-opaque marker band)
- ✓ A **puncture needle**
- ✓ A **J-guidewire**





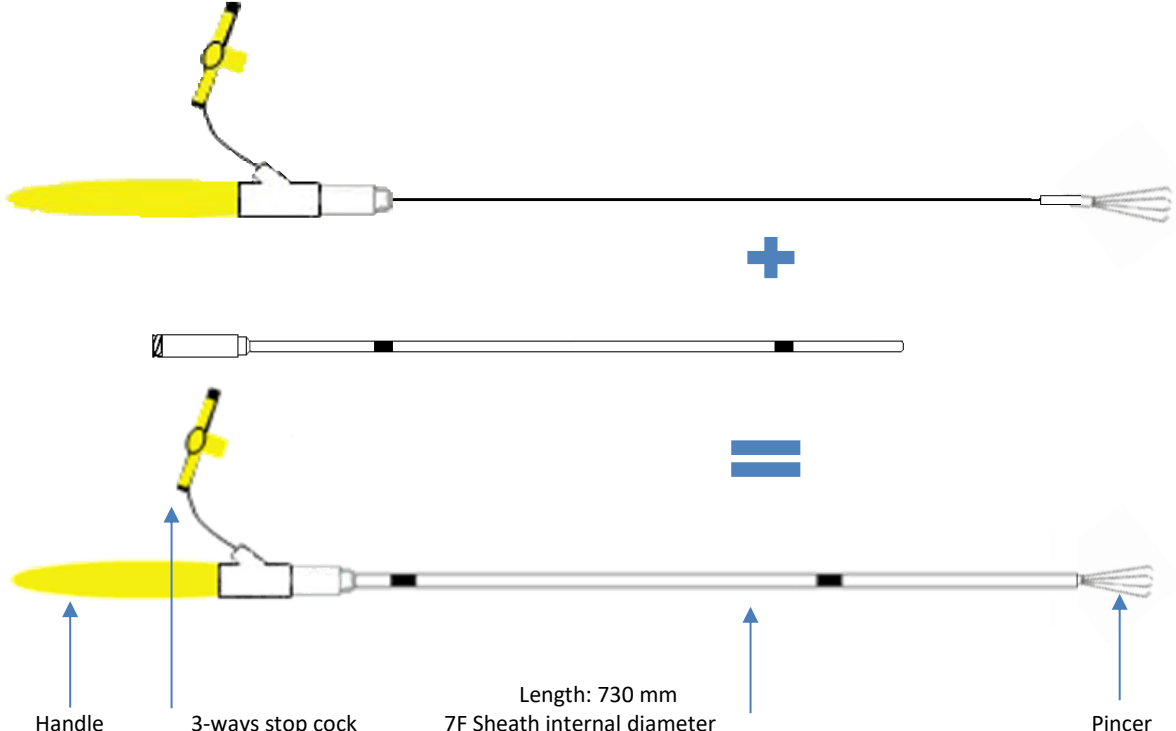



Parameters of the Retrieval System

Diameter of the strands (mm)	Material	Diameter of the pincer (mm)	Length of the pincer (mm)
0.4	Stainless 316 LVM*	13.5-15	24 

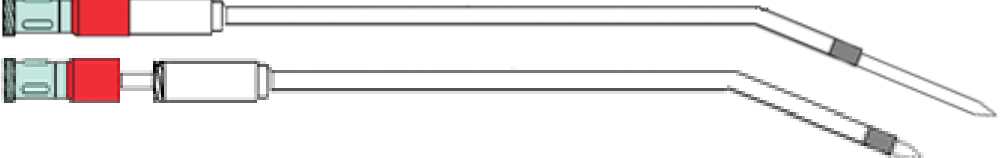



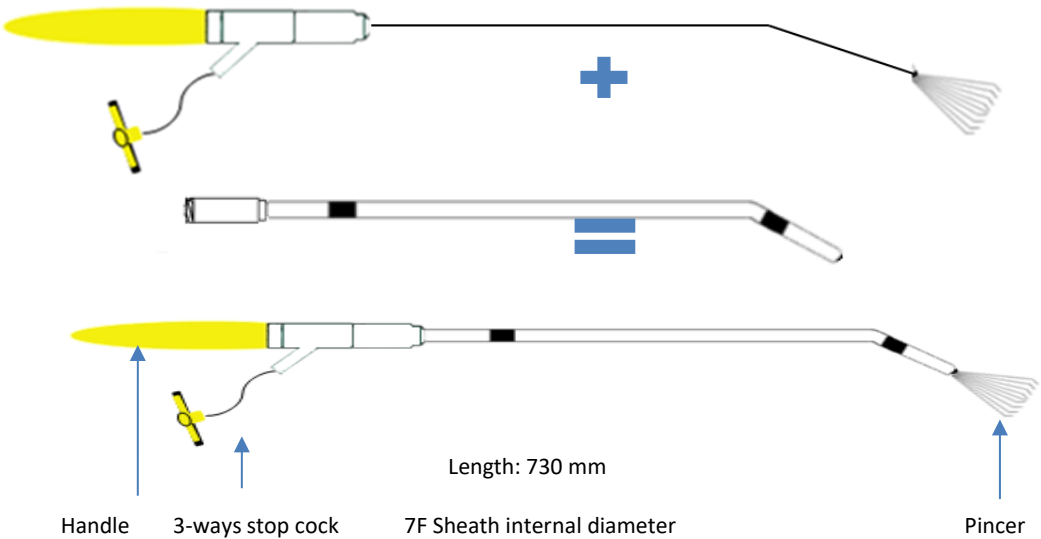


*ISO 5832-1

The ALN Extraction and/or Repositioning Kit ALN Straight RS

ALN STRAIGHT RS	
Approach	Jugular
Product Code	FT.902010
Introduction system: Dilator in the extraction sheath	
	
Extraction sheath	 <p>Radio-opaque marker band ————— \varnothing Internal: 9F Length: 570 mm No haemostatic valve \varnothing External: 11F</p>
Dilator	 <p>\varnothing Internal: 3F Length: 630 mm \varnothing External: 9F</p>
Sheath	 <p>Two black markers to visualize the stages of the removal procedure \varnothing Internal: 7F Length: 596 mm \varnothing External: 9F</p>
Pincer Kit	 <p>Length: 730 mm 7F Sheath internal diameter</p> <p>Handle 3-ways stop cock Pincer</p>
Puncture needle	\varnothing : 17 G
J-guidewire	<p>\varnothing : 0.035" J Radius (mm) : 3</p>  <p>Length: 150 cm</p>

Sterilization by ethylene oxide

The ALN Extraction and/or Repositioning Kit ALN Pre-curved RS

ALN PRE-CURVED RS	
Approach	Jugular
Product Code	FT.902010/VS2
Introduction system: Dilator in the extraction sheath	
	
Extraction sheath	 <p>Radio-opaque marker band No haemostatic valve</p> <p>Ø Internal: 9F Ø External: 11F</p> <p>Length: 570 mm</p>
Dilator	 <p>Ø Internal: 3F Ø External: 9F</p> <p>Length: 630 mm</p>
Sheath	 <p>Two black markers to visualize the stages of the removal procedure</p> <p>Ø Internal : 7F Ø External : 9F</p> <p>Length: 596 mm</p>
Pincer Kit	 <p>Length: 730 mm</p> <p>Handle 3-ways stop cock 7F Sheath internal diameter Pincer</p>
Puncture needle	 <p>Ø : 17 G</p>
J-guidewire	<p>Ø : 0.035"</p> <p>J Radius (mm) : 3</p> <p>Length: 150 cm</p> 

Sterilization by ethylene oxide

